



MiniMed™ 780G system changing the Silhouette® infusion set quick reference guide

Start here

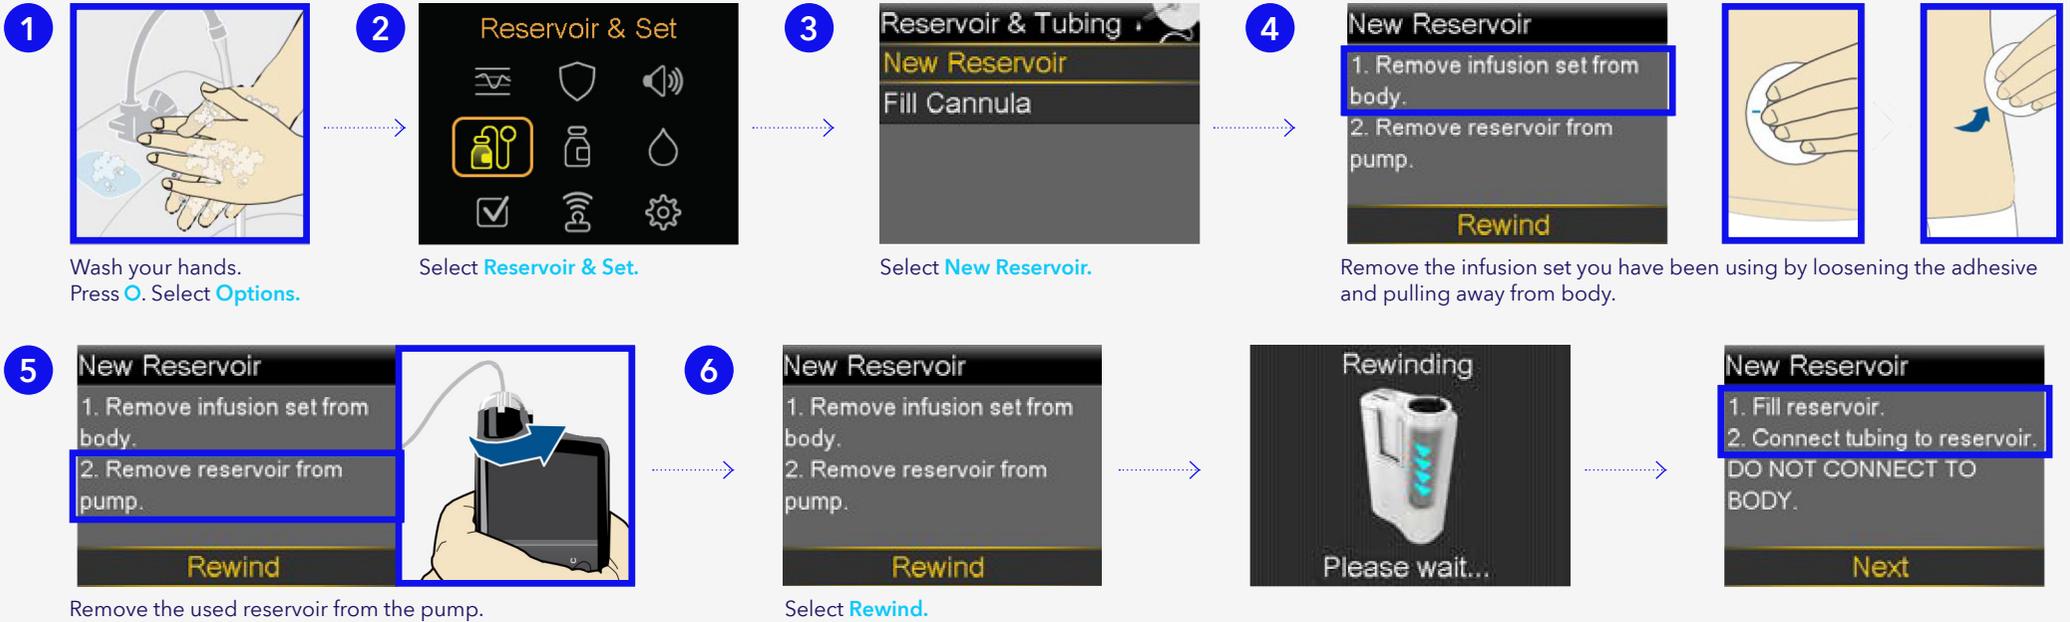


Fill reservoir & connect to the infusion set tubing

Follow the next steps to fill reservoir with insulin and connect to the infusion set tubing.

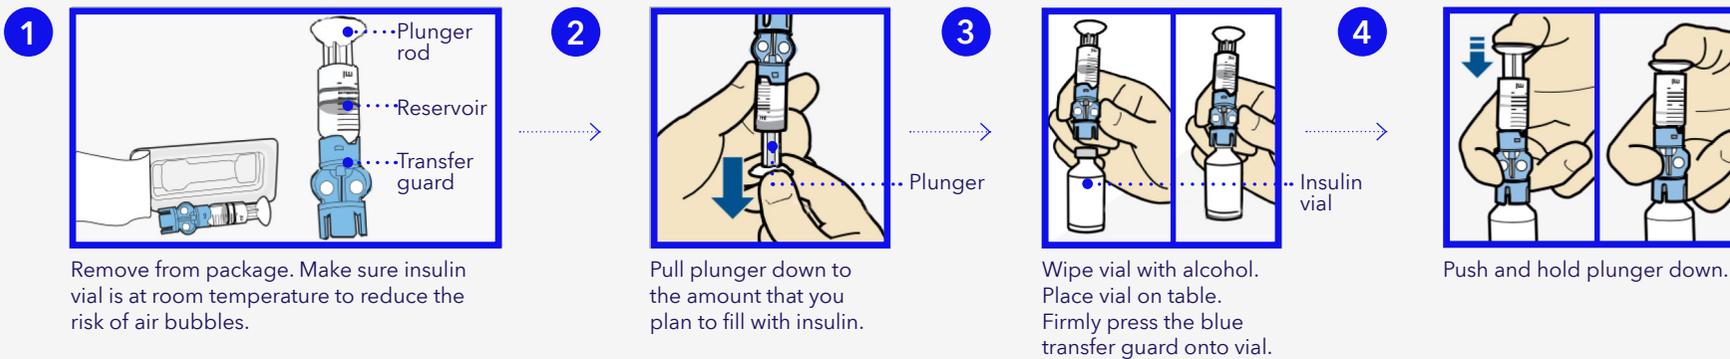


MiniMed™ 780G system changing the Silhouette® infusion set quick reference guide


! If insulin or any liquid gets inside the tubing connector, it can temporarily block the vents that allow the pump to properly fill the infusion set. This may result in the delivery of too little or too much insulin, which could cause hyperglycaemia or hypoglycaemia.

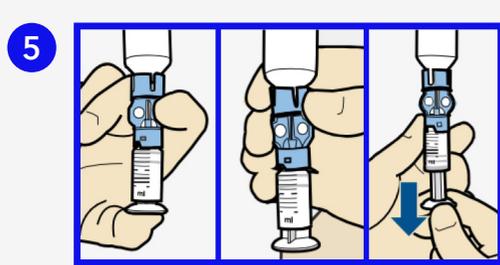


5 With your thumb still on the plunger, flip over so vial is on top. Release thumb and pull plunger down to fill with insulin.

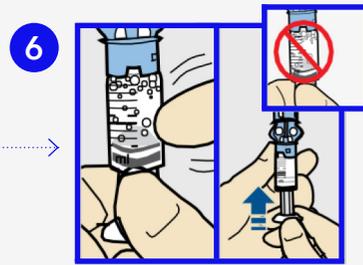

6 Tap the reservoir to move air bubbles to top of reservoir. Push plunger up to move air into vial.

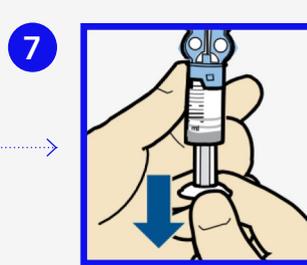


7 If needed, pull plunger back down to amount of insulin needed for 2-3 days.

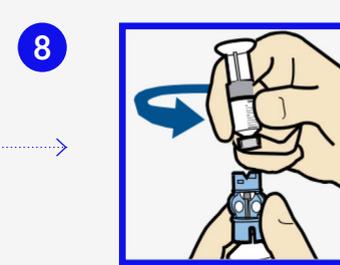


8 To avoid getting insulin on the top of the reservoir, turn vial over so it is upright. Hold transfer guard and turn reservoir counter-clockwise and remove from transfer guard.

Connect reservoir to infusion set


You will place the tubing connector onto the end of the infusion set to the filled reservoir.

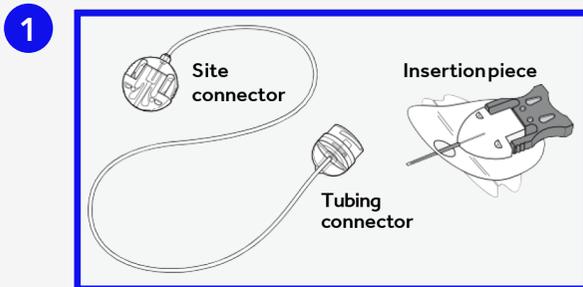


1 Remove infusion set from package. Remove the paper that holds the tubing together.

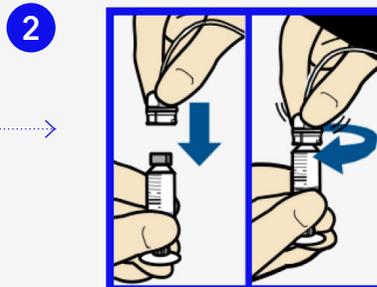

2 Gently push the tubing connector onto reservoir. Turn clockwise until locked. You will hear a click.

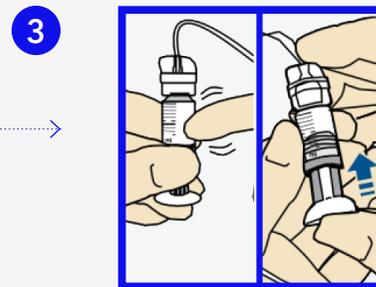

3 If you see air bubbles, tap reservoir to move them to top. Push plunger just a bit to move them into tubing.

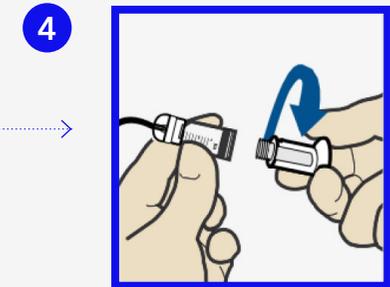

4 Twist the plunger counter-clockwise to loosen and remove.

The backlight may have turned off


Press any button to turn the screen back on.



1 Press **O** to open the menu.



2 Select

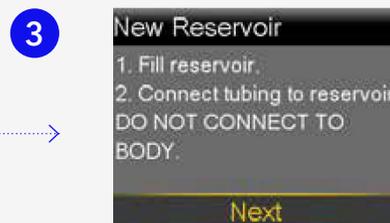


3 Select **Next**.


MiniMed™ 780G system changing the Silhouette® infusion set quick reference guide

Place reservoir into pump

Now place the filled reservoir into the reservoir compartment of the pump.

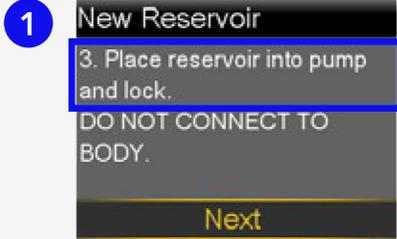- 

Place reservoir into pump.
- 
- 

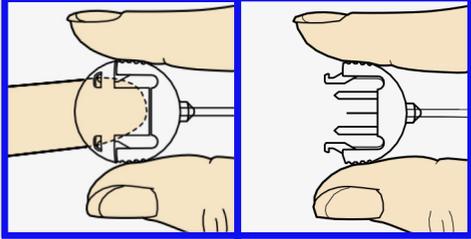Turn clockwise until you feel reservoir lock into place.
- 
- 


Select **Next**.


Load reservoir and fill tubing

Follow these steps to load the reservoir and fill the tubing.

- 

Select **Load** and keep holding **O**.
- 


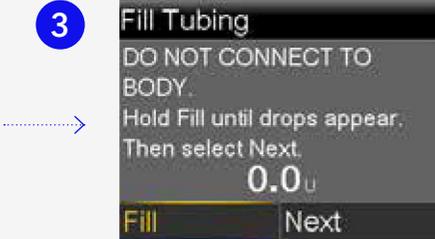
When you see this screen, select **Next**.
- 

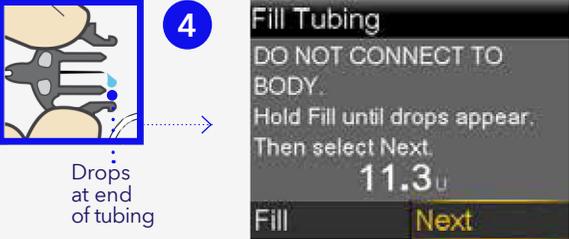Select **Fill** and keep holding **O** until you see drops at the end of tubing, then let go.
- 

After you see drops, press **>** and select **Next**.

Insert infusion set - two methods

Next, follow these steps to insert the infusion set into your body.

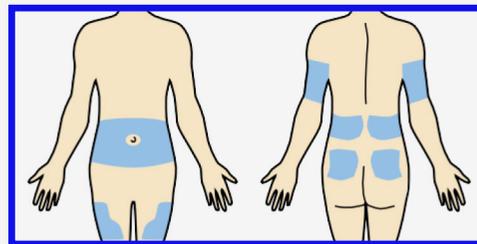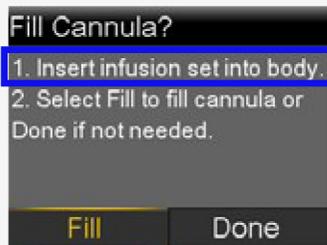

Choose an insertion site from the shaded areas shown here. Wipe with alcohol or other antiseptic.


.....> **Method 1:** Insertion By Hand.

.....> **Method 2:** Insertion Using The Sertter.

MiniMed™ 780G system changing the Silhouette® infusion set quick reference guide


Method one - by hand

1



Hold the insertion piece by the gray needle handle using the thumb and middle finger.

2




Hold the tape with your forefinger and remove the needle guard.

3



Pinch up skin at prepared site. Use other hand to insert needle at a 20-45° angle.

4

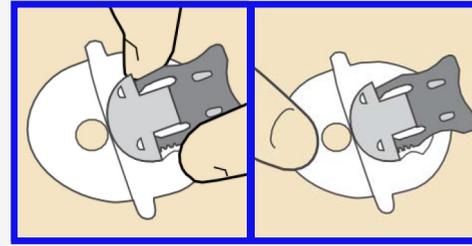


After it is inserted release the skin and hold inserted piece in place.



Action:
Proceed to the **Remove Introducer Needle** section.


Method two - using theserter

1




Use thumb to press down on the Lock & Release handle of theserter.

2




Place the insertion piece inside theserter and let go of the Lock & Release handle. Theserter prongs should fit securely into the holes of the insertion piece.

3




Use thumb to slide the Lock & Release handle back until you hear a click.

4




Gently pull off the needle guard.


5




Rest arms of theserter against skin so that it is at a 20-45° angle.




6




Press the white button at the top of theserter to insert the infusion set.



7




Hold infusion set against skin with one hand. With the other hand press the Lock & Release handle to open theserter. Then, slide theserter back from infusion set.





MiniMed™ 780G system changing the Silhouette® infusion set quick reference guide


Removing introducer needle

Next, follow the steps to remove the introducer needle.

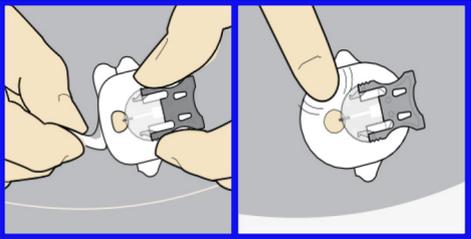- 

Peel paper from the front part of the adhesive and press adhesive securely to skin.
- 

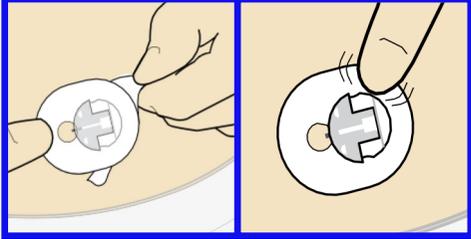
Squeeze arms on the gray needle handle & pull back to remove introducer needle.
- 

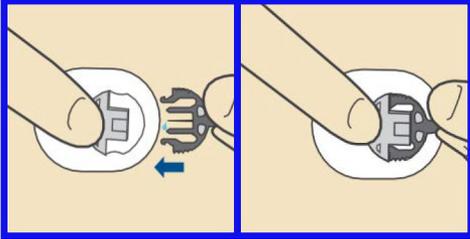Peel rest of the paper without lifting infusion set too far from skin. Press adhesive securely to skin. Dispose needle into a sharps container.
- 


Select **Next**.

Fill cannula

You will now fill the cannula, the little tube under your skin, with insulin.

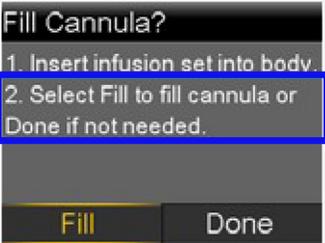- 

Select **Fill**.
- 

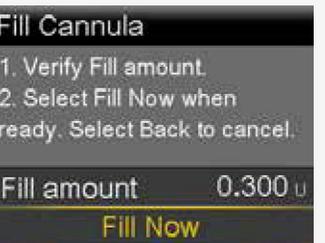Select **Fill amount** and enter:
⌚ 0.300 if using 6mm cannula
⌚ 0.500 if using 9mm cannula and press **⊙**.
- 

Select **Fill Now**.
- 

The Home screen displays the insulin as it fills the cannula.

i Note:
Your pump will remember the **Fill amount** that you used last. Always verify that the **Fill amount** is correct.

- ⌚ If it is correct, press **▼** to **Fill Now** and press **⊙**.
- ⌚ If it is incorrect, press **⊙**. Change to correct amount and press **⊙**. Select **Fill Now**.

i Note:
Select **Stop Filling** if you need to stop, for example, if you notice the **Total** amount is incorrect. This should rarely happen if you have verified the **Fill amount** on the previous screen.

Your infusion set change is now complete!